


<b>Title:</b> ALGORITHM FOR ASSESSMENT OF NEEDLE PLACEMENT/CATHETER PATENCY IN CVC DEVICES	<b>Number:</b> III-80
<b>Effective Date:</b> 01 January 2003	<b>Approved By:</b> Provincial Systemic Therapy Program

## Access CVC Device and Assess Blood Return

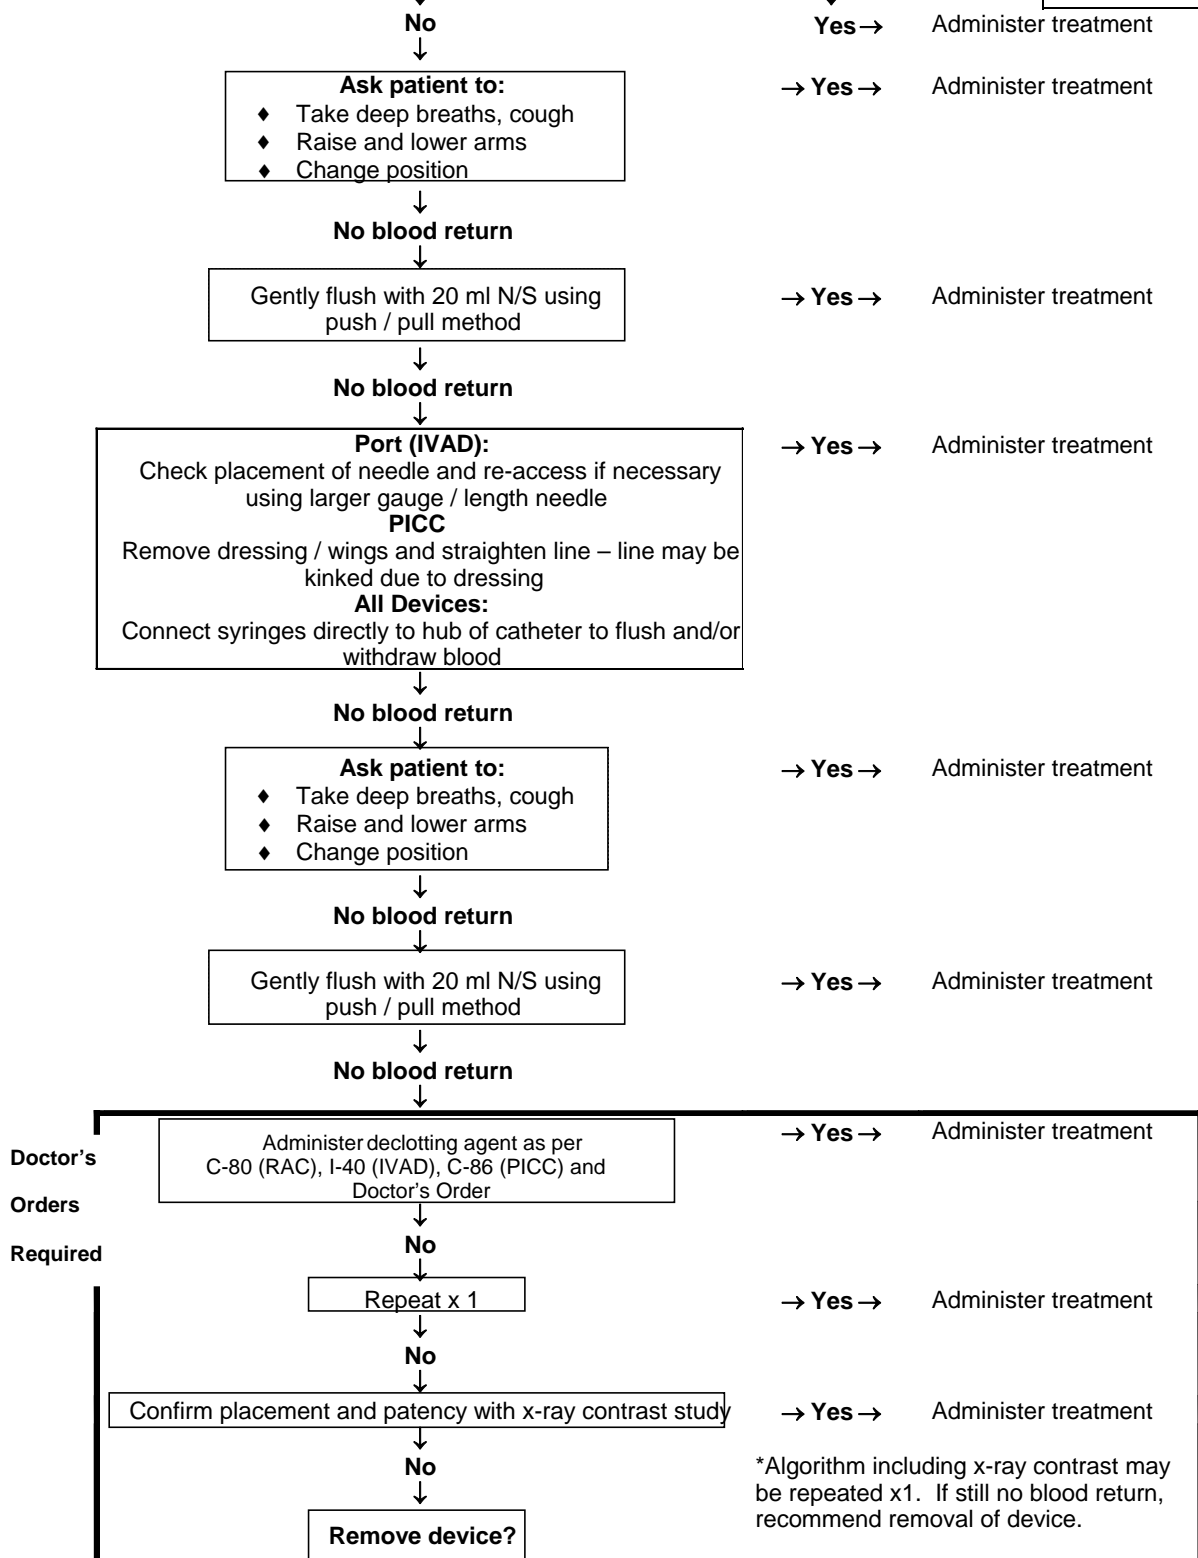

\*Algorithm including x-ray contrast may be repeated x1. If still no blood return, recommend removal of device.